Conversion Instructions

Content

1 Application 1
2 Included in the Kit 1
3 Instructions 1
3.1 General: 1
4 Final Testing 1
5 Figures 2

1 Application

This conversion kit is intended for the pneumatics module (M33999) in the Julian (8601110) anesthetic workstation. The extension plug —to be used on the PCB Ventdos-actuator and connected to the power cable— will change the way the sensor lines work (5-Volt connection).

Schutz nach DIN 34 beansprucht.
Use of the document / contents is forbidden without express authority. All rights reserved.
Dräger Medizintechnik GmbH, D-23542 Lübeck

2 Included in the Kit

This conversion kit contains the following:

1	Conversion Instructions	8604089
1	Extension Plug	8604084

3 Instructions

3.1 General:

Switch off the Julian anesthetic machine and remove the back panel.
Remove the power plug (orange plug) from the PCB Ventdos-actuator (8201921).
Connect the extension plug to the PCB Ventdos-actuator and reconnect the power plug.
Remount the back panel to the anesthetic machine.

4 Final Testing

Carry out technical safety checks and tests according to the corresponding Test Certificate.
Allow the power-on self test to be carried out.
Connect a test thorax and select IPPV.
Check the ventilation parameters.

5 Figures

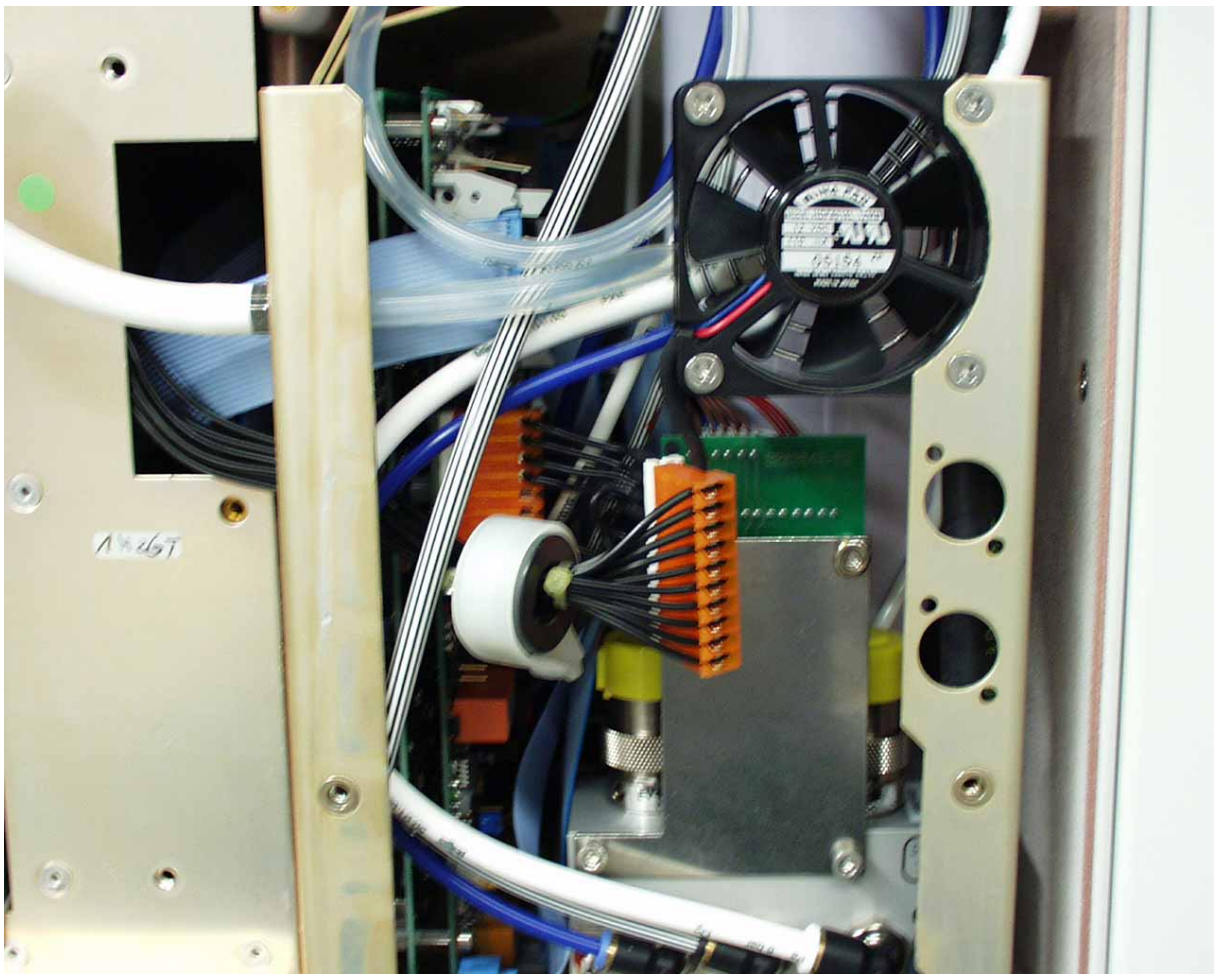

Schutz nach DIN 34 beansprucht.
Use of the document / contents is forbidden
without express authority. All rights reserved.
Dräger Medizintechnik GmbH, D-23542 Lübeck